


# APOS system check report: 11:42:26 07.09.2020

Apos GmbH  
Wedel



CSU:	1	Sample used:	Dyspro
Sensor:	1	TargetValue expected:	242,79
Source:	wood_water (5)	TargetValue received:	242,72

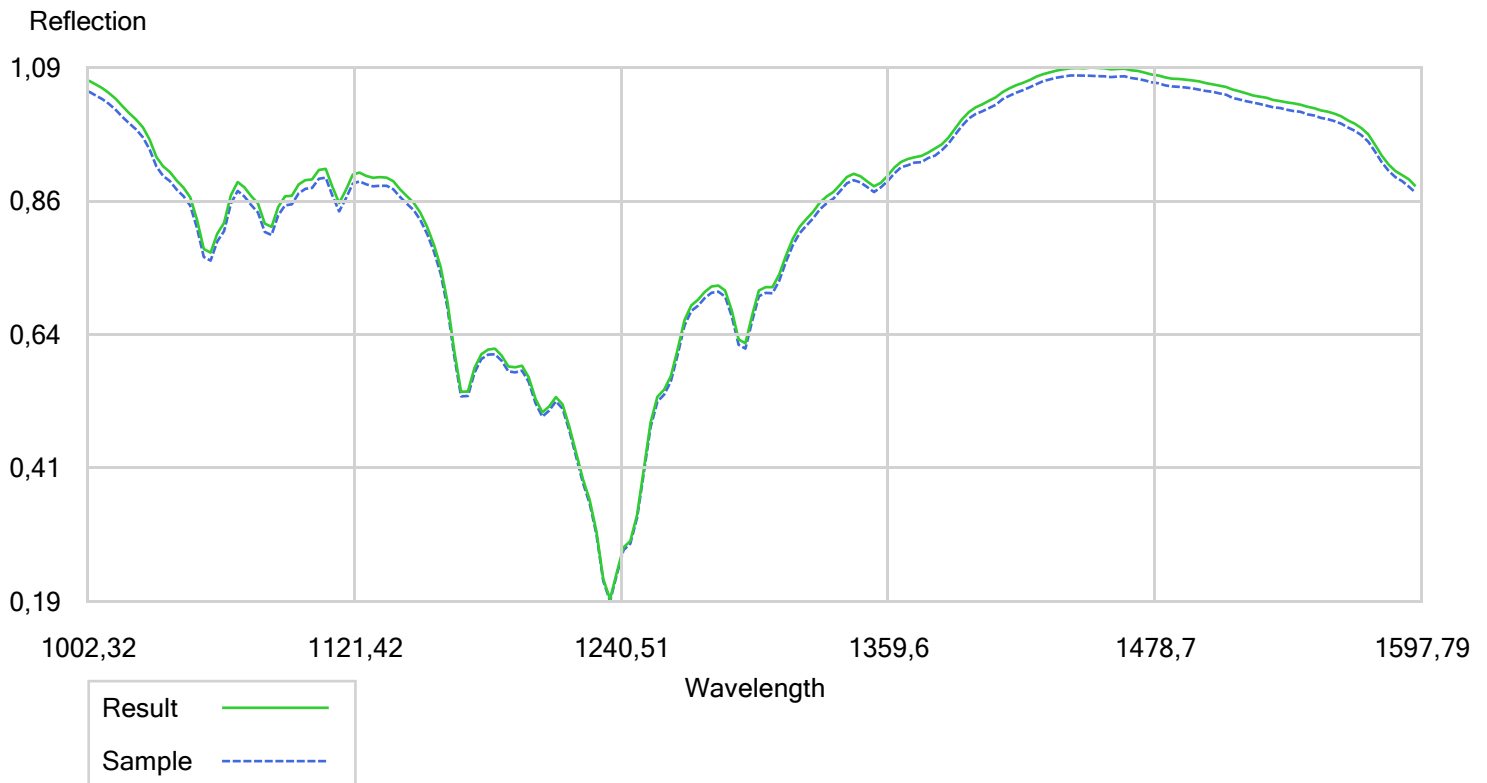

Successful

  
Am Marienhof 4  
D-22880 Wedel  
Tel.: +49 (0)4103-18783-0  
Fax: +49 (0)4103-18783-98  
info@apos.biz · www.apos.t